

THE NEUROSIGN V4

INTRAOPERATIVE NERVE MONITOR

PRESERVING NERVE INTEGRITY





 **NEUROSIGN[®] V4**






NOP18-EN-03
January 2021






CE
2797



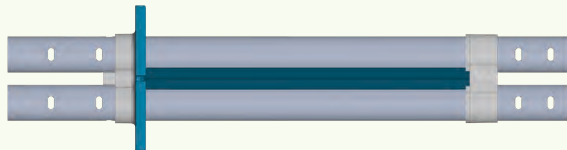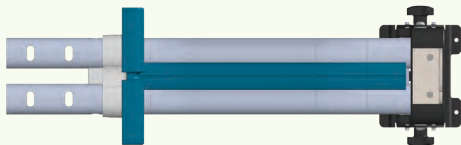

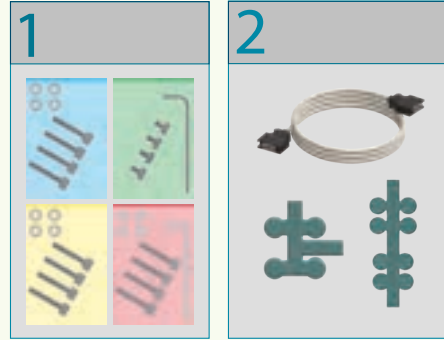

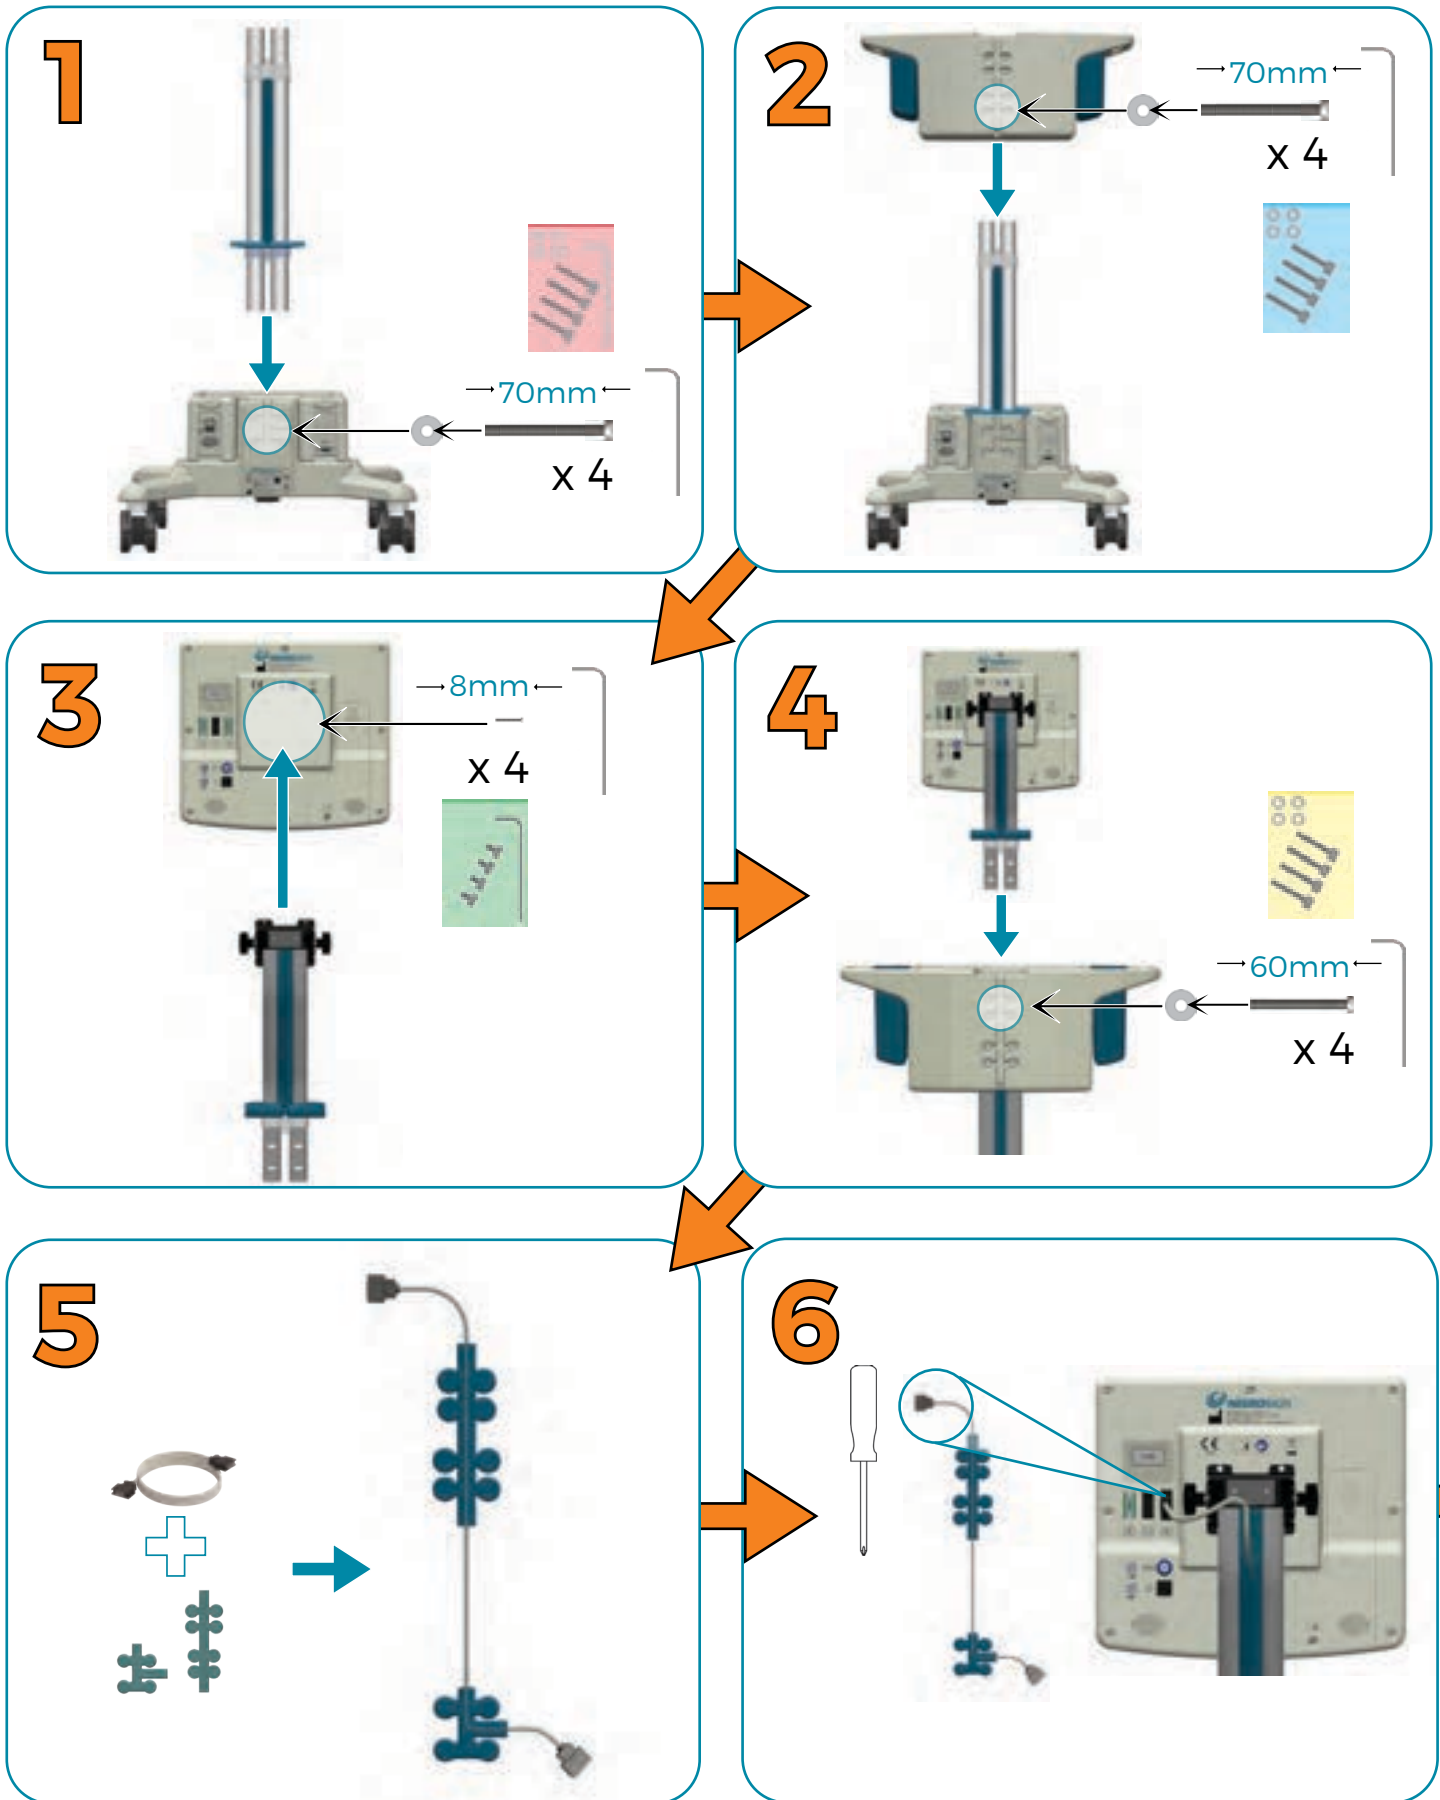

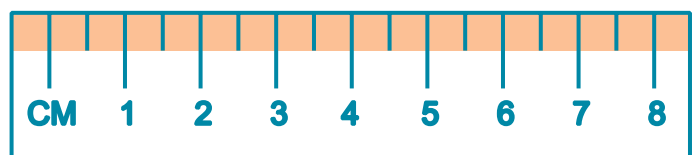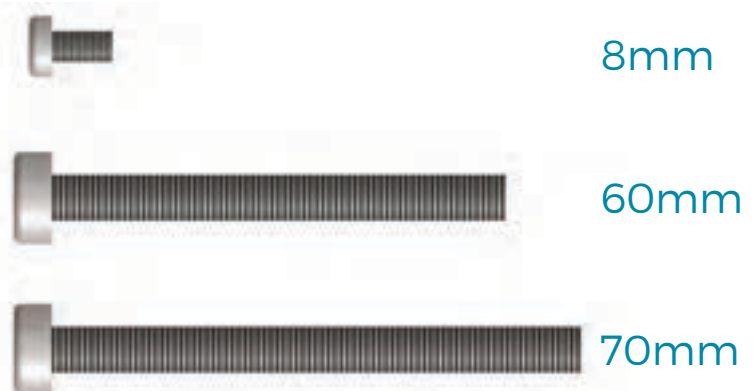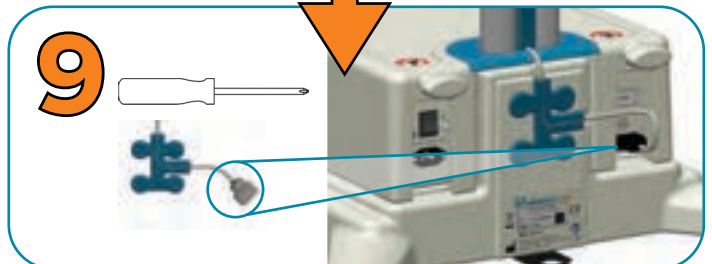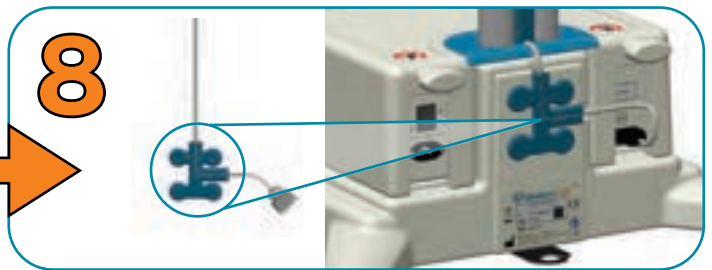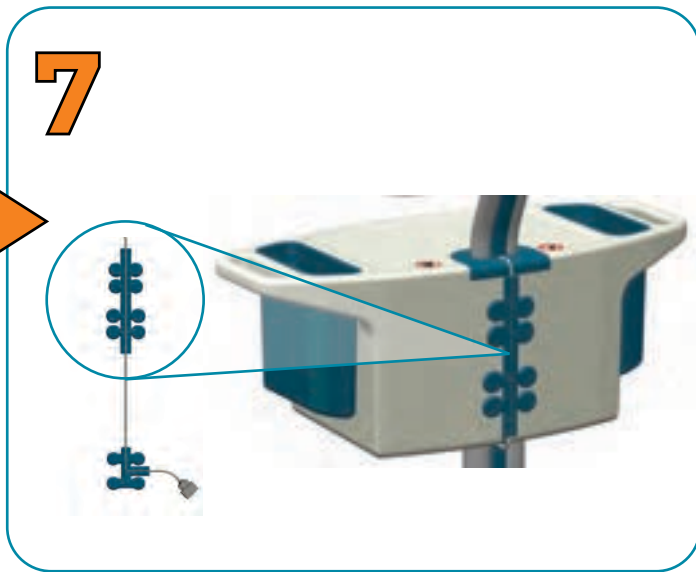




www.magstim.com



The Magstim Company Limited
Spring Gardens, Whitland, Carmarthenshire, SA34 0HR

 +44 (0)1994 240798

 +44 (0)1994 240061

 info@neurosignsurgical.com

 <http://www.neurosignsurgical.com>



Technomed Europe
Amerikalaan 71, 6199 AE Maastricht-Airport,
The Netherlands

 +31 43 408 68 68

This document should be considered along with the
Neurosign® V4 User Manual (NOPO8)

Copies are available from your local Neurosign representative